



Atomic Absorption Spectrophotometers





## AA-7000 Series

Atomic Absorption Spectrophotometers


## **Reaching Even Greater Heights**

Enhanced Flame Analysis World-Class High-Sensitivity Furnace Improved Dual Atomizer System Advanced Safety Technology



# System Configuration can Evolve with Your Needs

The AA-7000 Series can be upgraded by adding units to allow the system to handle the analysis targets.

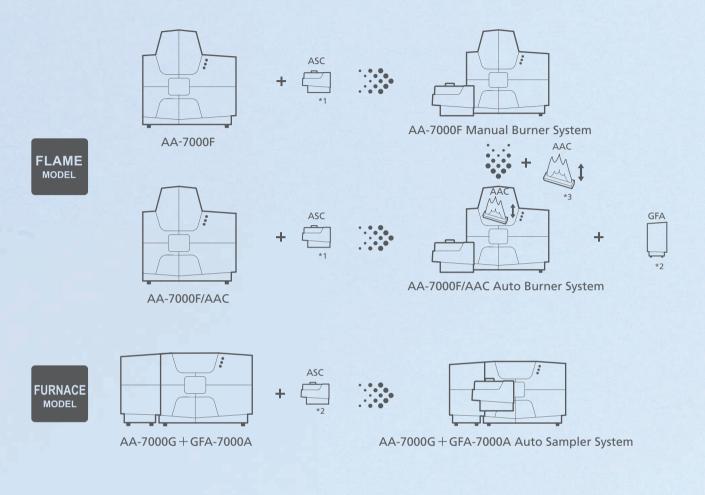

## **Major Fields of Application**

## **Analysis Sensitivities**

AA-7000 Series supports a wide range of analysis applications.



#### Environment

Seawater, river water, effluent, sludge, air-borne dust

Metals, Semiconductors, Ceramics Metals, minerals, glass, ceramics, IC chips



Petroleum, Chemicals, Polymers Petroleum, oil, catalysts, chemical products, biodiesel


Medical, Biology, Pharmaceuticals Blood, animals, plants, drugs, food products

									Flam	ime				Furnace			
												1			1	1	
	Concentration limit of detection								<0.01	0.01 ~0.09	0.1 ~0.9	1~		<0.01	0.01 ~0.09	0.1 ~0.9	
											(ppm)					(ppb)	
Η																	He
Li	Be											В	С	Ν	0	F	Ne
Na	Mg											Al	Si	Р	S	Cl	Ar
K	Ca	Sc	Ti	V	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr
Rb	Sr	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	Ι	Xe
Cs	Ba	La	Hf	Ta	W	Re	Os	Ir	Pt	Au	Hg	Tl	Pb	Bi	Po	At	Rn
Fr	Ra	Ac															
				Ce	Pr	Nd	Pm	Sm	Eu	Gd	Tb	Dy	Ho	Er	Tm	Yb	Lu
				Th	Pa	U	Np	Pu	Am	Cm	Bk	Cf	Es	Fm	Md	No	Lr


\* May differ according to coexisting substances in the sample.







#### AA-7000F/AAC Dual Atomizer System



Autosampler

AUTO 

Dual Atomizer System Automatic adjustment of atomizer Automatic serach of burner height

Flame and Measurement Procedures

- \*1 Requires ASC stand kit. \*2 Requires ASK-7000.

\*3 Automatic burner height search function can be used. AA-7000F/AAC equips with AAC as standard.

ASC

## **Flame Selection**

														Air-C2H2	N2O-C2H2	HVG	MVU
Η																	He
Li	Be											В	С	N	0	F	Ne
Na	Mg											Al	Si	Р	S	Cl	Ar
K	Ca	Sc	Ti	V	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr
Rb	$\mathbf{Sr}$	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	Ι	Xe
Cs	Ba	La	Hf	Ta	W	Re	Os	Ir	Pt	Au	Hg	Tl	Pb	Bi	Po	At	Rn
Fr	Ra	Ac															
				Ce	Pr	Nd	Pm	Sm	Eu	Gd	Tb	Dy	Ho	Er	Tm	Yb	Lu
				Th	Pa	U	Np	Pu	Am	Cm	Bk	Cf	Es	Fm	Md	No	Lr



AA-7000F Flame Model



AA-7000G Furnace Model (with options attached)



## **Enhanced Flame Analysis**



## **Double-Beam Optics and Stable Hardware Achieve Superior Stability**


The AA-7000 Series incorporates newly developed 3D double-beam optics.

The optical system has been designed to produce its maximum performance for each measurement method through optimal adjustment of the light beam and light beam digital filter, and by using optical components that restrict light losses.

## Advantages of the Double-Beam System


#### Long-term stability

The graph shows the results of measurements on 2 ppm copper (Cu) conducted over at least one hour. (The plot shows mean values for 11 repeated measurements.) Over the course of more than 600 measurements, the instrument achieved a relative standard deviation within 1%.



#### High sensitivity

The graph shows the direct measurement results for 0.1 ppm lead (Pb).



0.1 ppm to 0.4 ppm Calibration Curve for Lead (Pb)

11.110

nit filmer.

6.109

## Support for Developing Analytical Conditions

#### Automatic gas flow rate optimization

Automatic searching for optimal fuel gas flow rate (Japanese Patent 2099886). It is important to determine the optimal gas flow rate for the flame when using an organic solvent or after changing the burner height. The AA-7000F Series automatically optimizes the gas flow rate by measuring the changes in absorbance between a blank and a standard sample. The difference between the two is displayed on the screen. The gas flow rate achieving the highest sensitivity is detected and this value is automatically set as the gas flow rate value.

#### Automatic burner height optimization (AA-7000F/AAC)


The absorption sensitivity for flame analysis is also affected by the burner height. This results from variations in the flame temperature due to the burner height. The flame temperature is also affected by the matrix components. AA-7000F/AAC adjusts the burner height in 0.5 mm steps to automatically search for the optimal conditions.

AA-7000F enables above function by AAC-7000 (option).

## **Optional Autosampler Reduces Analysis Workload**

#### Low carryover

Great care must be taken to avoid carryover during flame analysis. The new ASC-7000 autosampler rinses the nozzle at the rinsing port on the overflow mechanism after each sample measurement is complete. This ensures 10<sup>-4</sup> max. carryover during the measurements of multiple samples. The graph shows the results of consecutive analyses of 10 ppm, 20 ppm, and 50 ppm sodium (Na) standard solutions in the EMISSION mode. No carryover could be detected when measuring the 10 ppm standard sample immediately after the measuring the 50 ppm Na standard sample.



Conventional method Overflow method

## Trace Sample Analysis Using Micro Sampling

#### Micro sampling

At least 1 mL (1000 µL) volume of a liquid sample is required for the continuous intake of sample during normal flame analysis. With micro sampling, however, approximately 50 to 90 µL of sample is injected in one shot into the flame and quantitation is based on the height and area of the peak signal obtained. This method offers the advantages below.


#### Advantages

- Permits analysis of small sample volumes
- Multi-element analysis of small sample volumes
- No blockage of burner slot with samples having a high salt concentration
- · Synchronized with the autosampler for auto-dilution measurements
- \* Synchronization with the autosampler requires the optional micro sampling kit.

#### Example of micro sampling analysis

Examples of the measured waveforms (overlaid) and calibration curve for micro sampling analysis are shown to the right.

A 2-ppm Cu standard solution was prepared by auto-dilution using the autosampler. The autosampler can also be used to conduct dilution measurements of the sample. (Injection volume: 90 µL)





## World-Class High-Sensitivity Furnace

## Achieves World-Class Lower Limits of Detection

Advances in optics and a new graphite furnace design achieve improved lower limits of detection for furnace analysis (comparison with previous Shimadzu models).

This superb analysis performance is possible in all fields.

Enhanced	Sensitivity	due to	o Graphite	Furnace
----------	-------------	--------	------------	---------

Previous	New
Pb 0.08ppb	<b>0.05ppb</b>
Mn 0.02ppb	<b>0.01ppb</b>

## **High-Performance Autosampler**

- Mix and inject up to four sample types (diluted solution, standard solution, sample, matrix modifier, etc.). (Of course, unmixed samples can also be injected.)
- Select a fluororesin tube or pipette tip as the injection nozzle.
- Automatic dilution and re-analysis if the calibration curve concentration is exceeded.




#### Example of Automatic Dilution and Re-Analysis


Analysis of cadmium (Cd): The maximum concentration of the calibration curve has been set to 1ppb. At 1.8ppb, the sample of [003] has exceeded the maximum concentration. As a resultit has been automatically diluted by 4 times and re-measured.

											-			
***	Action	Sample ID	True Value (ppb)	Conc. (ppb)	Ats	Pos	VOL	Diluent R1	Reasent 1 R2	Total Volume	ASC	Actual Conc.	Actual Gonc. Unit	Out of Control Remark
19	SPIREA 2	001+05	0.1300	10.768t	8.3059	4	10	1	2	20		17661	10.0	
20	SPIKELA	001+0	0.2500	0.7558	0.3049	4	10	5	5	20	1	0.7558	ppb	
21		1.0				2							1.00	
22		11-				1								
23	-	-				10	100	1 10	-	100			and a	
24	UNIC3-1	ODE.		0.5238	0.2128	*	3	45	g	20	4.0000	2.0924	ppb	
25	UNKS-3	003		0.3947	0.2050	2	3	15	11	28	4,0000	2.0158	pplo	
26	LINK3-AV	003		0.5138	0 2086	5	5	15	0	20	4.000	2 0552	ppb.	

### High-Sensitivity Application Data (Analysis of Selenium (Se))

Independent control of the gas flow through the graphite tube during atomization achieves extremely high-sensitivity measurements. (Japanese Patent 2067563)





Measurement Example Showing High Sensitivity

Analysis of 0 to 5 ppb selenium (Se): Sensitivity is adequate for 1 ppb measurements. (20  $\mu$ L injected volume, Pd modifier, pyro-coated graphite tube)

#### Digital temperature control and electronic gas flow control enhance stability

Combination of a high-sensitivity optical sensor and unique digital temperature control technology achieves highly accurate temperature control in all temperature regions from drying to atomization. An electronic flow controller can precisely control the inner gas flow rate in 0.01 L/min units. These control techniques significantly enhance both the sensitivity and the data stability.

#### Measurement Example Showing High Stability

Analysis of 0.5 ppb lead (Pb): Approx. 5% relative standard deviation after 5 repeated measurements is adequate for quantitative analysis.





High-density graphite tube (P/N 206-50587) Can be used for all elements. Especially effective for low-boiling point elements (Cd, Pb, Na, K, Zn, Mg, etc.).



**Pyro-coated graphite tube** (P/N 206-50588) Effective for elements that readily form carbides (Ni, Fe, Cu, Ca, Ti, Si, V, Mo, etc.).




#### Platform tube (P/N 206-50887-02)

Restricts chemical interference due to coexisting substances. Effective for the analysis of environmental samples and biosamples, such as sea water and industrial waste.

\* Depending on the state of the sample, some other combinations may be appropriate.



## Improved Dual Atomizer System

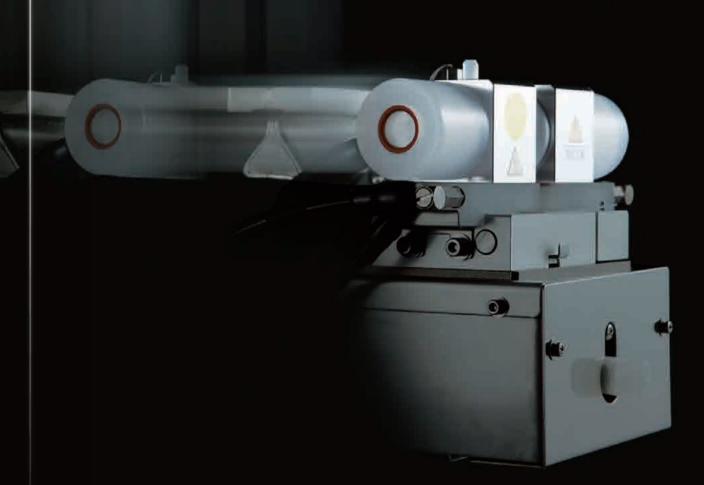

## Single Unit Handles High Concentration to Trace Analysis Samples

AA-7000F/AAC creates an integral burner and furnace that remains permanently installed in the combustion chamber. It supports both flame analysis of high concentration samples and furnace analysis of trace samples, without changing the atomizer unit. The integral construction with the atomizer saves space. AA-7000F enables above function by AAC-7000 (option).

\* The AAC-7000 cannot be attached to an AA-7000G instrument.

### New Atomizer Design Permits Easy Switching Between Flame and Furnace Measurements


- The new drive mechanism halves the switching time between flame and furnace measurements (comparison with previous Shimadzu models).
- The atomizer unit is switched automatically by software operation. No troublesome replacement of the atomizer unit is required. No need to disconnect pipes or wires.
- In case of the flame measurement of high-concentration sample, offsetting the burner head from the light axis, instead of angle adjustment, allows to adjust the sensitivity.
- A single autosampler can be used for both flame and furnace measurements. Simply slide it left or right. No need to purchase two autosamplers.



#### Smallest footprint for a full system

The system with a dual atomizer fits into a 960 mm width (including power supply for the graphite furnace atomizer), achieving the world's smallest installation footprint\* for a full system.

\* Shimadzu in-house investigation. Current as of November 2008.

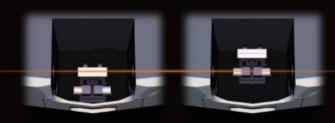

Flame measurement: Burner head intersects the light axis (red line).

Furnace measurement: Furnace intersects the light axis (red line).



Flame measurement



Furnace measurement

#### Easily attach an autosampler

Direct connection of the autosampler to the AA instrument minimizes the installation footprint and simplifies maintenance.




#### Lamp house

Just slide the cover to the side for easy replacement of the hollow cathode lamps through the large opening.







\* Dimensions do not include ASC-7000. Height (H) does not include protrusions.




## Advanced Safety Technology



## **Comprehensive Safety Functions in Every System**

Safety is an extremely important consideration for flame atomic absorption spectrophotometers using acetylene gas. The AA-7000 Series instruments are the first\* ones in the world fitted with a vibration sensor as standard. They also incorporate a comprehensive range of safety mechanisms, including gas leak detectors.

\* Shimadzu in-house investigation. Current as of November 2008.

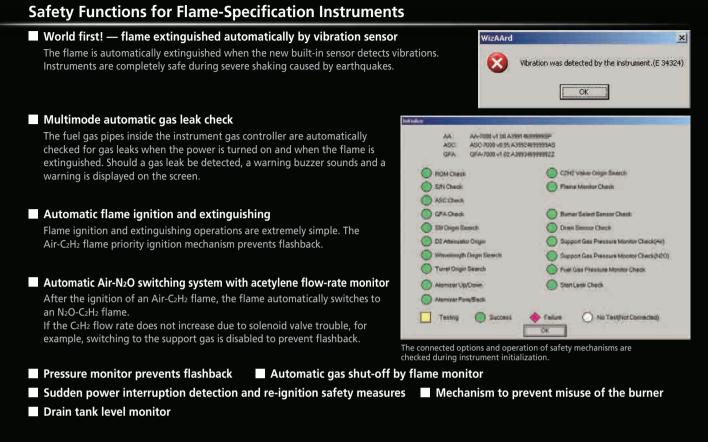

## Safety Functions for Furnace-Specification Instruments

- Cooling water flow rate monitor Argon gas pressure monitor Furnace cooling check
- Overcurrent protection unit (double-checked by circuit protector and optical sensor)

## Safety-Conscious Design

#### Flame-retardant materials

UL 94V-0-rated flame-retardant materials are used for the instrument external covers and atomizer unit. This superior design pays due consideration to safety.

#### Safe ignition switches

The switches perfectly fit finger contours and are positioned near the window. To prevent inadvertent operation, both switches must be

pressed simultaneously to start ignition.

## Durable pipes and reliable couplings

All pipes are selected for durability and used with highly reliable couplings.

#### Clear window

The large window permits observation of the flame, and the burner can be easily accessed through the large opening. The window closes when released to eliminate the chance of it being left open.







## **Dual-Background Correction Functions**

The optimal background correction methods are installed as standard: high-speed self-reversal method (SR method) and deuterium lamp method (D<sub>2</sub> method).

These functions can correct for spectral interference in flame measurement. Selecting the optimal background correction method for each sample ensures accurate and reliable analysis results.

Samples suitable for the SR method


Samples with a complex matrix (Containing a large quantity of a specific element as the main component) Samples suitable for the D2 method

Purified water, tap water, environmental water, etc. Samples with a relatively simple matrix

### SR (high-speed self-reversal) method — accurate background correction over a wide range

#### **Features**

- 1. High-speed self-reversal (SR) correction is generally more accurate than deuterium lamp (D<sub>2</sub>) correction. As both atomic absorption and background absorption can be measured using a single lamp, the correction errors due to light-axis misalignment are extremely small. This is ideal for the quantitation of trace components in a matrix exhibiting complex background absorption, such as bio-samples and metals.
- 2. Permits background correction over the entire wavelength range from 185 nm to 900 nm.
- 3. This method can correct for spectral interference due to neighboring lines that can occur when a resonance line for another element exists near the analytical line for the target element. (See table on next page.)
- 4. As no polarizer is used, measurements are possible with low light losses and a high S/N ratio.
- 5. The rapid lamp lighting permits accurate measurement unaffected by emission noise in the atomizer.
- \* Hollow cathode lamp L-2433 is required to use the SR method. Hollow cathode lamp L-2433 can also be used for the D2 method.

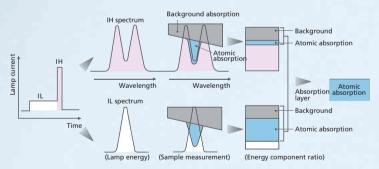

#### Principle

A small current IL (approx. 10 mA) and a large current IH (approx. 500 mA) are alternately passed through the hollow cathode lamp. The lamp emission spectrum when the large current flows has a depression in the center (self-reverse), due to self-absorption of the large number of sputtered atoms in the atom cloud, as shown in the diagram to the left. No significant atomic absorption is apparent and background absorption mainly occurs. Conversely, the lamp emission spectrum when the small current flows comprises a single narrow peak resulting from both atomic absorption and background absorption. By determining the difference between the two types of absorption, it is possible to accurately correct for the background absorption and measure the true atomic absorption.

① Zn 0.25ppm

2 Zn 0.50ppm


⑤ Fe 0.5% +Zn 0.25ppm ⑥ Fe 0.5% +Zn 0.5ppm

⑦ Fe 0.75% +Zn 0.3ppm


③ Fe 0 1%

④ Fe 0.5%

**Examples suitable for SR method (where differences result between SR and D**<sup>2</sup> **methods)** Example: Measurement of trace levels of zinc in iron (analysis of Zn in Fe solution)

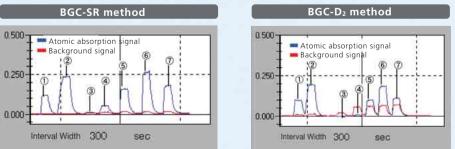

The identical 0.5 ppm Zn solution is accurately corrected to the same absorbance at (2) and (6).



<b>Examples of</b>	elements	and	wavelengths causing spectral
interference	problems	due	to neighboring lines


<b>Measured Element</b>	Analytical Line (nm)	<b>Coexisting Element</b>	Absorption Line (nm)
AI	309.28	Mg	309.30
As	193.76	Fe	193.73
Ca	422.67	Fe	422.64
Cd	228.80	Ni	228.84
Cu	324.75	Fe	324.73
Ga	294.36	Ni	294.39
Mg	285.21	Fe	285.18
Ni	232.00	Fe	232.04
Pb	217.00	Fe	216.95
Sb	217.58	Fe	217.55
Se	196.03	Fe	196.05
Si	251.61	Fe	251.69
Zn	213.856	Fe	213.8589
Zn	213.856	Fe	213.8589

The SR method is suitable for samples containing elements that cause problems with spectral interference, as shown in the table to the left.

## D<sub>2</sub> (deuterium lamp) method — highly sensitive background correction

#### **Features**

- 1. Detection sensitivity is superior to the SR method. Therefore, this method is suitable for the analysis of samples with a simple matrix requiring high sensitivity, such as the measurement of trace levels of impurities in ultrapure water or environmental analyses.
- 2. As the lighting frequency is higher than with the SR method, it can eliminate noise due to emission components of the flame or graphite tube to permit accurate atomic absorption measurements.
- 3. The original hollow cathode lamp can be used.




#### Principle

The deuterium lamp method involves lighting the hollow cathode lamp and the deuterium lamp alternately at high speed. After separation by the monochromator, the light from the deuterium lamp has a bandwidth from 0.1 to 5 nm. Therefore, an atomic absorption with a line width of only about 1/1000 nm is almost unobservable compared to the background absorption due to wide-bandwidth molecular absorption. However, as the light from the hollow cathode lamp has approximately the same bandwidth as the atomic absorption band, the total of the atomic absorption and the background absorption can be observed. With the deuterium lamp (D<sub>2</sub>) method, light from both sources passes through the atomizer. The difference in absorbance is determined to conduct background correction.

#### Examples suitable for D<sub>2</sub> method (where no difference results between SR and D<sub>2</sub> methods)

Example: Measurement of trace levels of lead in 2% NaCl solution by molecular absorption (analysis of Pb in 2% NaCl solution)

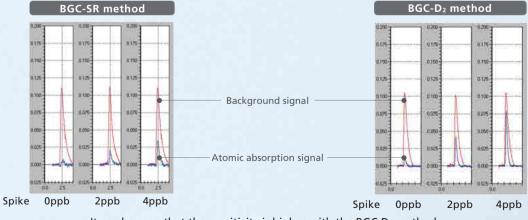


It can be seen that the sensitivity is higher with the BGC-D<sub>2</sub> method.

## AA-7000 Series Clear, Easy-to-Use Software


### Features of the WizAArd Software

The WizAArd software used with the AA-7000 runs under Windows 7/Vista/XP.

Wizard Functions Make Setting the Conditions So Simple That Even a Novice Can Do It.

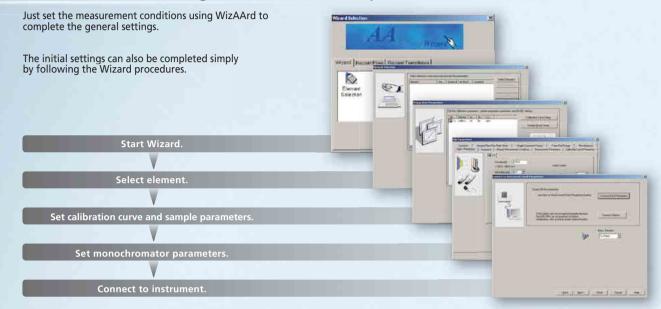

## Measurement Screen Layout Shows Measurement Status at a Glance

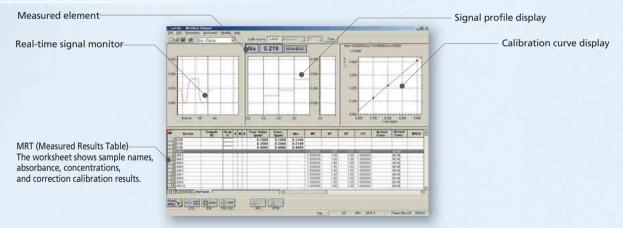

## Lamp History Function Assists with Lamp Management


The accumulated operation time for each lamp displayed on the lamp registration screen assists with lamp service life management. Multiple lamps for the same element are differentiated using lamp IDs.

	Lamp 10	Dement	Lamp Type	Life Time	tiund Time	Unit	Judge	Comment	Lock	Of.
1.	02		02	500	0.0	hri	OK		F -	TANALTZ
2	Ap.1	Ag	Normal	5000	0.0	mAYEE	OK		E	Cencel
¥.	AL1	A	Normal	5000	0.0	mAthra	OK		E	
4	An-1	At.	Northek	3000	68	matten	OH		E	Clear
4 5	ALLS:	Au	Normal	5000	00	mAttra	OK		E	
6	B-1	6	Norrial.	5000	0.0	1156.900	CH		E	Delete
7	Be-1	Ba	Namal	5000	0.0	mAfre	OH			- BENNING
1	Be-1	De	Namia	5000	10.0	mAtra	OK		E I	200
£1	DI-1	13	Northill	5000	0.0	mA'res	Cas		E L	Ennt
10	Ca-1	Ca	Northill	8000	0.0	mates .	CHK		E	
112 112	Cdift	Ca	Noribik	5000	0.0	mAmro	OH		E	
12	Covt	Co	Norrow	5000	0.0	matris	QWE		F	
13	Cr-F	de .	Normal	5000	0.0	mAtres	CHK		F	
14.	Ct-1	Ca	Normal	5000	0.0	matters	CH		E I	
15.	0.61	-T.84	Alternati	9000	0.0	matters	06		11	

### Software Provides Comprehensive Information Displays and Flexible Settings


### Identical software operation for flame and furnace measurements

- Even if the calibration curve is created after sample measurements, concentration calculations can be conducted on past data. This allows trial measurements to be directly used as actual measurements.
- Extrapolation of calibration curve range. If the sample concentration exceeds the calibration curve range, additional measurements can be performed on standard solutions to re-calculate the concentration.
- Ose existing calibration curves for measurements. Useful for sample concentration order checks and for checking the instrument sensitivity.
- ④ One-touch re-measurement operation. No need to repeat the measurement from the beginning.
- Create and save multiple calibration curves on a single worksheet. Select the appropriate calibration curve for the sample concentration and composition.

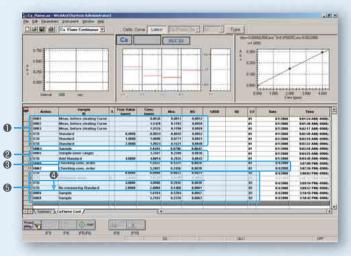

### Combining a high-performance autosampler simplifies advanced settings

- Real-time drying and ashing progress display for furnace measurement
- A higher temperature cleaning operation than the cleaning stage can be added for each measurement. This reduces the graphite tube memory effect. Tube deterioration is reduced by minimizing the cleaning operations.
- SAdd optional autosampler rinsing operations to ensure adequate rinsing of the autosampler after completing the measurement of high-concentration samples.
- ④ Set up sample dilution and spike-and-recovery tests on the same screen.
- **(5)** Overlay function allows size and shape comparison of peak profiles.
- **6** Large-volume injection permits high-sensitivity measurements.
- Precision control of drying and ashing temperatures reduces analysis time.

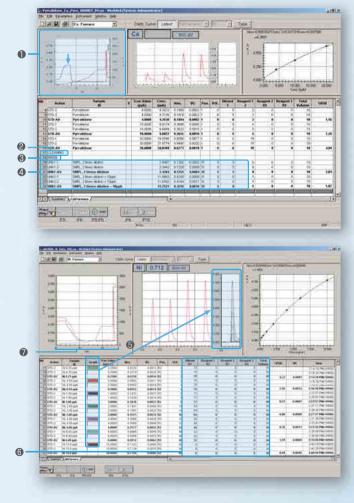

## **Supports System Management and Accuracy**

## FDA 21 CFR Part 11 Compliance

AA-7000 Series

- A combination of enhanced WizAArd software with Shimadzu's network-compatible CLASS-Agent data management software supports FDA 21 CFR Part 11 Compliance.
- WizAArd used alone provides comprehensive system policy setting, user management, log browser, audit trail, and electronic signature system management functions.
- Hardware validation software installed as standard.

determine how each one uses the

software.

### **Comprehensive Data Management Functions**

stem Policy e system policy settings allow advanced ssword and lockout settings. The levels n be set in stages from "unrestricted" "Part 11 compatible".	<b>CLASS-Agent (Option)</b> Connection to CLASS-Agent permits efficient, long-term database management of large amounts of analysis data.
Police Police	
Setting	
Minimum Pastword Length D days Prenament 8 set to Maximum Dataword Are D days C flataments south meet complexity requirements Lockout Settings for PC	
Login Attempt Land 11 The United of set for 01 Lockow Deadlon 115 The min	
Lockov Settines for Liner Lockov Settines for Liner Lockov System 15 3 min .	
# of Levels for Deplicate Parament () =	
	Validation System Policy Agent Competition Setting
	And a second secon
scaword   Users: Groups   Group Name Description 2 HW Adm, Extrument Configuration, Control and Adjustm. 2 Method De. Method Development	User Administration Log Browser
assword   Users Groups   Group Name Description 28 HW Adm Estrument Configuration, Control and Adjustm. 28 Method De. Method Development	User Administration Log Browser
Add <u>Promovo</u>	User Administration Log Browser User Administration Log Browser Sector Statement Tor Foreign Administration I like New Palance New Adjuster New Adju

The log browser easily displays a variety of logs to check the system modification history and other log information.

## Management

Accuracy Management (QA/QC) Functions Permit User Level Management, Audit Trail, and Electronic Signatures


QA/QC compatibility The QA/QC functions permit accuracy management.

et.		1.60	11		
IDA/DON	1.0000	HC NC	20	1 0	0
Method	True Value	· Par	VCH.	Disest	Hester13
<b>Departure</b> free	anataria.				
008,001	Fiegantic)	-	Liveyis	W = 1720	minuteitti
IF COB		IN CROK	- F	Mark & Co	nizue j
P.00V	90	*- p+0	K 0	Mark # Go	n)init ( S
N NE		CE CROL	. 6	Mark & Go	nthui 🦷
R IEV	10	R-Pto	58 F	Markill Co	ntinue
DESTV	Application	Louis Lie	a 17 10 0000	UDARS	the second second
F NTY	20	** 1905	<u>8</u>	Mark & Go Paule	interpression of
PICORE		0.642		Mark & Co	100 C
0.6/00 Tate	- Ancepta	nce Criter	a Detty		Alleri Action



#### Hardware validation software installed as standard

The hardware validation software makes it simple to evaluate the instrument performance. When combined with the autosampler, it automatically determines the wavelength accuracy, noise level, baseline drift, absorbance and repeatability, and prints out the results of comparison with the pass criteria.

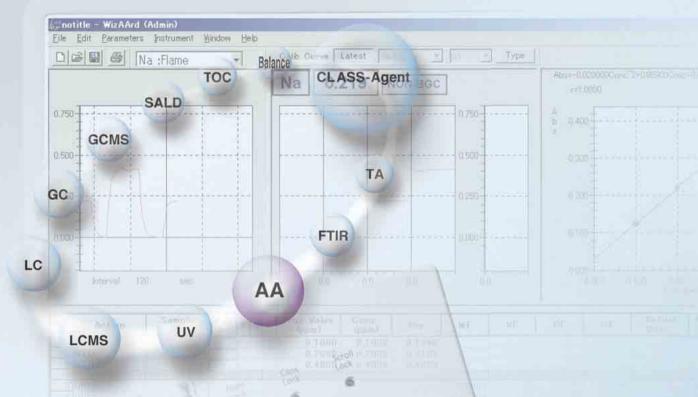

\* Data from all Shimadzu analytical instruments can be centrally managed by CLASS-Agent.



## AA-7000 Series Standard Parts / PC / Software

### **Common to All AA-7000 Series Models**

Part Name	Quantity	P/N
Cable set	1	071-60821-08 (120 V), 071-60825-51 (230 V)
Cards (set of 10)	1	206-52046-91
Instruction manual	1	206-97176
Safety inspection sheet (safety instruction)	1	206-97225
Declaration of conformity, explanatory notes (ISO-9001)	1	228-30164
Warranty label	1	037-70238-01
Registration form	1	221-40500
Serial number label	3	206-57770

\* The PC, monitor, printer, hollow cathode lamps, high-temperature burner head, pressure regulator and compressor are not included in the standard configuration.

## AA-7000F, AA-7000F/AAC Standard Parts List

Part Name	Quantity	P/N
Hose ASSY (for air supply)	1	206-50389-91
Hose ASSY (for C <sub>2</sub> H <sub>2</sub> gas supply)	1	206-50389-92
Hose clamp (16 mm)	2	037-61019
Cleaning wire	1	201-79229-01
Sampling tube (PTFE)	2	204-05899-01
Sampling tube (for organic solvent samples)	1	206-50772-91
Polyethylene tubing, No. 3	1 (0.3 m)	200-31328-01
Polyethylene tubing, 8 × 1 (drain tubing)	1 (2.4 m)	016-43201-02
Drain ASSY	1	206-77413-41
Grease (in cup)	1	206-50442-91
Funnel	1	206-77243-92
Declaration of conformity, English version (ISO-9001)	1	206-84934-66/-68
Inspection report	1	206-77551-02/-22

## **AA-7000G Standard Parts List**

Part Name	Quantity	P/N
Declaration of conformity, English version (ISO-9001)	1	206-84934-67
Furnace mounting plate	1	206-77704
Inspection report	1	206-77551-12

\* GFA-7000A is not included in the standard configuration.

### **Personal Computer / Monitor**

Microsoft Windows 7 Professional (32 bit) Vista Business or XP Professional
Intel® Celeron 420 (1.60 GHz) or higher
1 GB or higher (Vista) or 512 MB or higher (XP)
XGA (1024 × 768 dots) or higher
One CD-ROM drive (for installing software) Requires 60 MB min. hard disk space for installation
One serial port (for AA control)

\* Windows is a registered trademark of Microsoft Corp., U.S.A.

## **Optional Accessories**

## For Flame Analysis

Part Name	P/N	Remarks
High-temperature burner head	206-77530-91	Made of pure titanium. Air-cooled. 5 cm slot for N2O-C2H2 flame
T	~	• Extremely corrosion-resistant • Can also be used for Air-C2H2 flame.
Flow meter kit	206-77617-41	Float-type flow meter for support gas
Sample platform	206-77655-91	Dimensions: 250 W × 130 D × 170 H mm Vial mounting platform: 220 W × 95 D mm Vial positions: 5-step switching
Air compressor	208-91753-91	100 VAC, 50/60 Hz, with mist separator
Low-noise air compressor	208-91750-36	100 VAC, 50/60 Hz, with mist separator
Mist separator kit	206-52458-91	Required if using an air compressor other than above.
YR-71 compressed gas regulator	040-72020-01	For C <sub>2</sub> H <sub>2</sub>
MAF-85S compressed gas regulator	040-72019-11	For dinitrogen oxide gas
Micro sampling kit	206-77540-91	Required to use the flame micro sampling method. ASC-7000 and ASK-7000 (or ASC stand kit) are also required.
O-ring set	206-77620-92	O-ring set for organic solvents

## For Furnace Analysis

Part Name	P/N	Remarks
GFA-7000A graphite furnace atomizer	206-77777-XX	■ Specifications
	3	<ul> <li>Heating control system: Drying: Digital current control         <ul> <li>(with automatic temperature calibration function)</li> <li>Ashing, atomization: Digital temperature control via optical sensor</li> </ul> </li> <li>Heating temperature range: Ambient to 3000 °C</li> <li>Inner gas type: Dual automatic switching type</li> <li>Inner gas flow rate: 0 to 1.50 L/min, 0.01 L/min increments</li> <li>Ar gas: 3.5 L/min max.</li> <li>Cooling water: Cooling water circulation unit or tap for process water Water temperature: 10 to 30 °C, flow rate: 0.6 to 1.5 L/min</li> <li>* Separately order the parts below.</li> </ul>
Graphite Furnace Camera GFA-TV	206-52950-41	Provides viewing inside the graphite tube. Including Video View Software (CD-ROM)
High-density graphite tube	206-50587-11	
Pyro-coated graphite tube	206-50588-11	Select one of the three types of graphite tubes according to the aim of the analysis
Platform tube	206-50887-02	
MAF-106S compressed gas regulator	040-72019-21	For Argon gas
CA-1115A-1 cooling water circulation unit	044-01813-01	For cooling GFA, 100 VAC, 1100VA, 50/60 Hz
Parts for cooling water co	nnections	
Cooler connection kit	206-84373-41	For connecting GFA and CA-1115A-1
	206-51028-41	Connecting tubes when using tap water to cool GFA
Cooling water tube ASSY	200 31020 41	

## Autosampler

Part Name	P/N	Remarks
ASC-7000 autosampler	206-77600-XX	Specifications
For flame analysis	For furmace analysis	System: Flame / furnace Function: Zero-point detection, auto rinse, auto diagnosis, random access Maximum reagent / sample positions: Reagents: 8 positions, samples: 60 positions * Separately order the parts below.
ASC stand kit	206-77650-41	Required to mount ASC-7000 to conduct flame analysis only.
ASK-7000 extension unit for furnace analysis	206-77550-41	Permits both flame and furnace analysis.
Nozzle ASSY, HVG	206-67563	Required to use ASC-7000 and HVG-1.



## **Optional Accessories / Related Products**

## **Dual Atomizer System**

Part Name	P/N	Remarks
AAC-7000 auto atomizer changer	206-77701-41	Required to add GFA-7000A to AA-7000F to conduct furnace analysis. Permits automatic burner position setting for flame analysis with AA-7000F.

## **Hollow Cathode Lamps**

Part Name	P/N	Remarks
L-233 series	200-38422-XX	
L-2433 series	200-38456-XX	For SR method

## **Other Accessories**

Part Name	P/N	Remarks
Analog output cable	206-77707-91	Used for analog output to a pen recorder, etc. One cable required per channel (atomic absorption/energy signal, background signal).

## For High-Sensitivity As, Se, Sb Analysis

Part Name	P/N	Remarks
Part Name P/N 206-17143-XX		<ul> <li>Environmental standards prescribe the hydride generation method as one method of As, Se, and Sb analysis.</li> <li>1. Used with the AA-7000 Series, HVG-1 permits the rapid and accurate quantitation of elements such as As, Se, Sb and Hg at several-ppb levels.</li> <li>2. Used with an ASC-7000 autosampler, it permits the automated serial analysis of up to 60 samples.</li> <li>* Nozzle ASSY, HVG (PN: 206-67563) is required to use HVG-1 with an ASC-7000 Series instrument. Order separately.</li> </ul>
	10	■ Specifications Measurement method: continuous flow Sample consumption: 0 to 7 mL/min, variable Reagent consumption: 0 to 2.5 mL/min, variable Atomizer: Heated absorption cell (heated by Air-C:H2 flame in standard system) Carrier gas: Ar pressure: 0.32 MPa, consumption: 70 mL/min Power requirements: 100, 120, 220, 230, 240 VAC, 35 VA, 50/60 Hz Dimensions: 340 W × 220 D × 200 H mm Weight: Approx. 9 kg
-		■ Standard Major Items Hydride vapor generator, absorption cell (P/N: 206-77607) Reagent bottles (P/N: 206-58792-40/-42), gas hose, drain tube, etc.

## For Higher Sensitivity with the Hydride Generation Method

Part Name	P/N		Remarks
SARF-16C atomic muffle furnace (Electronic Cell Heater) 208-97249		hydride vapor 2. The temper temperature. 3. Good temp damage due t	ted furnace permits higher sensitivity measurements using the r generator than the flame heating method. ature controller provides optimal control of the quartz cell erature reproducibility. Extends cell life by preventing to overheating. (ffler cannot be used when an AAC-7000 is installed on an AA-7000F/AAC ons Dimensions: 170 W × 110 D × 110 H mm I.D.: o25 × 170 mm
		Controller * Use a stepdown	Heater: PYROMAX DS Operational temperature range: Ambient to 1100 °C Temperature regulation range: ±2.5 °C Load capacity: 1000 W max. Power requirements: 100 VAC, 400 VA, 50/60 Hz n transformer in regions that do not have a 100 V power supply.
	206-52135-91	For AA-7000F	
Mounting adaptor	206-83755-91	For AA-7000G	

## For High-Sensitivity Hg Analysis

Part Name	P/N	Remarks
MVU-1A mercury vaporizer unit	206-58780-XX	<ul> <li>This mercury vaporizer unit permits analysis using the reduction vaporization — atomic absorption method. It permits easy, high-sensitivity water quality analysis.</li> <li>Specifications</li> <li>Vaporization method: reduction vaporization with a reducing agent Measurement method: recirculation</li> <li>Flow cell: optical path length 100 mm (with quartz window)</li> <li>Sample volume: 250 mL max.</li> <li>Exhaust contamination prevention: adsorption trapping in mercury trap bottle Dimensions: 310 W × 357 D × 288 H mm</li> <li>Weight: Approx. 10 kg</li> <li>Standard Major Items</li> <li>MVU-1A unit: 1</li> <li>Reaction vial (P/N: 200-93018-01): 5</li> <li>Reaction vial lid (P/N: 204-21989): 2</li> <li>Stirrer tip (P/N: 046-00617-06): 10</li> <li>Mercury trap bottle (P/N: 206-58777-42): 1</li> <li>* Separately order the parts below.</li> <li>Gas flow cell (P/N: 206-77703-91)</li> <li>Holder for gas flow cell (P/N: 203-8422-28)</li> </ul>

## **ICP Emission Spectrometers**





## AA-7000 series Specifications

## Main Unit

### Basics

	Wavelength range	185.0 to 900.0 nm
	Monochromator	Aberration-corrected Czerny-Turner mounting, Number of grating grooves: 1800 lines / mm, Focal length: 300 mm
	Bandwidth	0.2, 0.7, 1.3, 2.0L nm (4-step automatic switching)
	Detector	Photomultiplier tube
Optics	Optics	Optical double-beam
	Background correction method	BGC-SR (high-speed self-reversal method) (185.0 to 900.0 nm)     BGC-D2 (D2 lamp method) (185.0 to 430.0 nm)
	Number of HC lamps	6-lamp turret, 2 lamps simultaneously lit (1 for measurement, 1 warming up for next measurement)
	Lamp mode	EMISSION, NON-BGC, BGC-D <sub>2</sub> , BGC-SR
	Software requirements	Microsoft Windows 7 Professional / Vista Business / XP Professional
	Parameter setting	Wizard method
	Measurement mode	Flame continuous method, flame micro sampling method, furnace method, flame emission method
	Concentration computation mode	• Calibration curve method (select primary, secondary, tertiary) • Standard addition method, simple standard addition method (primary expressio
	Repeat analysis	Up to 20 repetitions. Mean value, standard deviation (SD) and coefficient of variation (RSD) display Automatic exclusion of deviant values by setting SD and %RSD
	Baseline correction	Automatic correction of baseline drift by offset correction in peak height / peak area modes.
	Signal processing segment setting	Signal processing segments can be changed in peak height / peak area modes.
	Sensitivity correction	Automatic calibration curve correction function using sensitivity monitoring
Data Ar processing	Analog output	2 channels (atomic absorption/energy signal, background signal) Output range: 5.0, 2.5, 1.25, 0.625 Abs./V (each settable in 4 stages) Fixed at 1 V F.S. in EMISSION mode.
	Tabular data processing	Final concentration calculations based on sampled volume, dilution rate, fixed volume, and factor inputs
	Recall of parameters	Template functions available
	Procedure/result display	MRT (Measurement Results Table) worksheet
	Report generation	Summary report
	QA/QC	Select whether to continue or discontinue measurements based on results of evaluation on coefficient of correlation, %RSD, ICV·ICB, CCV·CCB, PB, LCS, SPK, PDS, and DUP.
	Re-analysis	Select whether on not to conduct re-analysis.     Automatic dilution and re-analysis of unknown samples via autosampler (flame micro sampling method, furnace method)
		Management by login ID and password      Control user access authority by user level
	Digital recording	• Log record • Audit trail • Electronic signatures
Power requ	lirements	Choose from 100, 120, 220, or 230 VAC, 50/60 Hz (Power is required separately for the personal computer.)
	s and weight	•AA-7000F/AAC: 700 W × 588 D × 714 H mm, 76 kg •AA-7000F: 700 W × 588 D × 714 H mm, 73 kg •AA-7000G: 700 W × 580 D × 538 H mm, 66 kg (Protruding parts and optional equipment are not included.)
Ambient te	mperature / humidity	10 to 35 °C, 20 to 80% (less than 70% when temperature is higher than 30 °C)

### Flame

	Туре	Air-cooled pre-mix type	
	Burner head	Titanium 10 cm slot (5 cm titanium slot for N2O-C2H2 flame available as an option)	
	Nebulizer	Pt-Ir capillary     •PTFE orifice     •ceramic impact bead (capable of handling hydrofluoric acid)	
	Chamber	Engineering plastics	
Burner unit	Positioning Angle adjustment	AA-7000F     Lateral/vertical manual adjustment     AA-7000F/AAC	
		Automatic flame/furnace switching by motor · Automatic search of optimum burner height     0 to 90° (Angle adjustment is not possible if the optional GFA-7000A is installed on the AA-7000F/AAC.)	
	Туре	Air-C2H2 flame, N2O-C2H2 flame (Hydrogen flame is not applicable)	
	Flow rate control	•Automatic fuel gas flow rate setting (0.1 L/min step) • Automatic search of optimum gas flow rate	
Gas control	Safety measures	Automatic gas leak check • Automatic Air-N2O switching as C2H2 flow rate increases • Flame monitor • Prevention of wrong burner head use     Gas pressure monitor • Drain tank level monitor • Automatic flame extinction upon power outage or sudden power interruption     • Automatic flame extinction via flame vibration sensor • Internal fan stop sensor	

## Furnace (GFA-7000A)

Heating temperature range	•Ambient to 3,000 °C	
Heating control system	Drying: Digital current control with automatic temperature calibration function     Ashing, Atomization: Digital temperature control via optical sensor	
Setting heating conditions	• Maximum 20 stages • Heating mode: RAMP/STEP • Inner gas type: Dual automatic switching type • High-sensitivity mode setting • Enrichment in furnace: Maximum 20 times • Optimum temperature program search support function • Inner gas flow rate: 0 to 1.50 L/min	
Safety measures	Cooling water flow rate monitor • Gas pressure monitor • Overcurrent protection unit (double check by circuit protector and optical sensor)     • Furnace block cooling check	
Positioning	•AA-7000G • Lateral/vertical manual adjustment •AA-7000F/AAC • Automatic flame/furnace switching by motor	
Power requirements 200, 220, 230, or 240 VAC ±5%, 7400 VA, 50/60 Hz		
Dimensions and weight	260 W × 560 D × 510 H mm, 47 kg	

## **Autosampler**

#### **Common Specifications**

Control	RS-232C communication control from AA unit	
Maximum reagent / sample positions	Reagents: 8 positions Samples: 60 positions (random access available with reagents or samples)	
Rinse water bottle	21	
Power requirements	Choose from 100, 120, 220, or 230 VAC, 50 VA, 50/60 Hz	

#### **Flame Continuous Method**

Functions	Zero-point detection, auto diagnosis, auto rinse, random access	
Sample volume	Sample vials: 15 mL, reagent vials: 53 mL	
Nozzle rinse	Solvent rinse aspiration method	
Dimensions and weight	Sampler: 340 W × 280 D × 270 H mm, 8 kg Controller (including stand): 260 W × 200 D × 320 H mm, 7 kg	

#### Furnace Method / Flame Micro Sampling Method

Functions	Zero-point detection, auto diagnosis, auto rinse, auto mixing, random access	
Sample volume	Sample vials: 2 mL, reagent vials: 20 mL	
Nozzle rinse	Solvent rinse discharge method	
Sampling functions	Dilution function, reagent addition function	
Syringe	250 µL	
Injection volume	2 to 90 µL	
Repeatability	1%RSD (20 µL)	
Carryover	Rinse port: Less than 0.0001 Mixing port: Less than 0.00001	
Mixing port rinse	Solvent rinse discharge method, solvent discharge and rinse with next sample	
Mixing function	Performed in mixing port. Maximum mixture volume: 0.6 mL	
Maximum number of mixing reagents added	Up to 4 solutions Number of solutions possible for mixing ·Calibration curve method: 5 solutions max. (sample + 4 types of reagents) ·Standard addition method: 6 solutions max. (sample + standard solution + 4 types of reagents)	
Auto dilution / re-analysis	For measurement result on unknown samples: If extrapolation of calibration curve is possible: automatic calculation of dilution rate and dilution to bring concentration within calibration curve range If extrapolation of calibration curve is not possible: dilution rate fixed at 10x	
Dimensions and weight	Sampler (including sliding parts): 340 W × 280 D × 400 H mm, 11 kg Controller: 235 W × 110 D × 240 H mm (built into GFA-7000A), 6 kg	

#### **Required Software Operation Environment**

Shimadzu recommends the PC and monitor in the PC Set for AA-7000 Series with WizAArd Software Pre-Installed. Purchase a printer separately. The personal computer and monitor specifications are as follows.

Operating system	Microsoft Windows 7 Professional (32bit) / Vista Business / XP Professional	
СРИ	Intel® Celeron 420 (1.60 GHz or higher) To use GFA-TV, Intel® Pentium DualCore E2180 (2 GHz) or higher is required.	
RAM	1 GB or higher (Vista) or 512 MB or higher (XP) To use GFA-TV, 1 GB or higher (GFA-TV)	
Monitor	XGA (1024 × 768 dots) or higher	
Storage device	One CD-ROM drive (for installing a software) Requires 60 MB min. hard disk space for AA installation.	
I/O port	One serial port (for AA control) USB 2.0 port (for GFA-TV)	
Peripheral device	Monitor, keyboard, mouse, printer	

\* Notes

•The PC, monitor and printer are not included in the standard configuration. Prepare them separately.

•The ASC-7000, ASK-7000 and GFA-7000A are optional accessories.

 $\cdot The separately available micro sampling kit is required for the flame micro sampling method.$ 


Microsoft Windows 7 Professional / Vista Business and XP Professional are registered trademarks of Microsoft Corp., U.S.A.

The AA-7000 Series does not conform to IEC60601 — Medical Electrical Equipment.



## **Installation Conditions**


## Dimensions

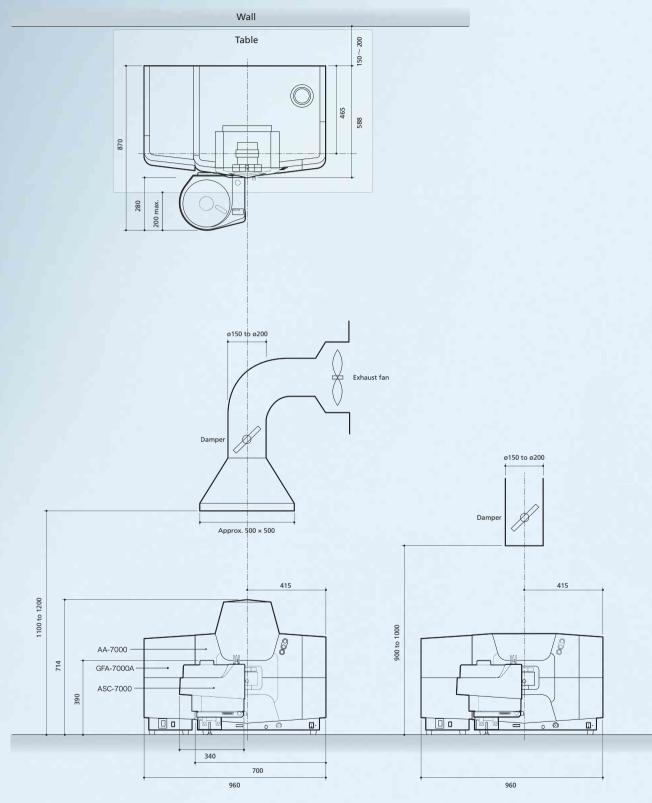


Both for flame analysis and furnace analysis

For furnace analysis

Make sure all required equipment is available before starting instrument installation. See the installation guidelines for details.



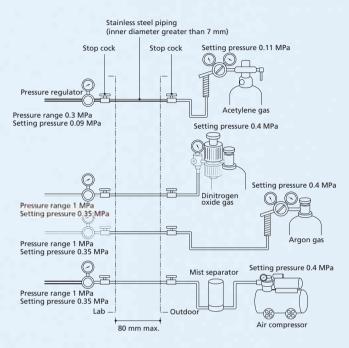

Temperature range	10 to 35 °C
Humidity range	20 to 80% (less than 70% when temperature is higher than 30 $^\circ \text{C}$
	1500 mm min. (W) × 700 mm min. (D)
	Withstand load: 200 kg *1, 2
Material	Stainless *3
Dimensions	7 mm min. I.D. × 80 mm min. (L)
A	Cylinder: 0.11 MPa
Acetylene	Lab: 0.09 MPa
	Compressor: 0.4 MPa
Air	Lab: 0.35 MPa
	Cylinder: 0.4 MPa
Dinitrogen oxide	Lab: 0.35 MPa
Argon	Cylinder: 0.4 MPa
	Lab: 0.35 MPa
Material	Stainless
Dimensions	For flame: Approx. 500 mm W × 500 mm D
	For furnace: ø150 mm to ø200 mm
In the last states	For flame: 600 to 1200 m³/hr
птаке сарасіту	For furnace: 10 to 180 m³/hr
(GFA-7000A)	Cooling water circulation unit or tap-water equipment *
	Humidity range Material Dimensions Acetylene Air Dinitrogen oxide Argon Material Dimensions Intake capacity


\*1 Atomic absorption spectrophotometer stand recommended

\*2 Maintain a free maintenance space of 150 to 200 mm to the sides and rear of the instrument.
\*3 Do not use pipes containing copper, silver, gold, mercury (or alloys containing these metals) as pipes for acetylene.

\*4 If tap-water equipment is used, ensure that it meets the specifications below.

Compatible faucet	Faucet 13 or 12 to 15 mm O.D. rimmed faucet
Water temperature	10 to 30 °C
Water flow rate	0.6 to 1.5 L/min
Supply pressure	0.08 to 0.15 MPa *5
Supply port	7 mm min.

\*5 If the supply pressure exceeds 0.17 MPa, use the optional Regulator ASSY.

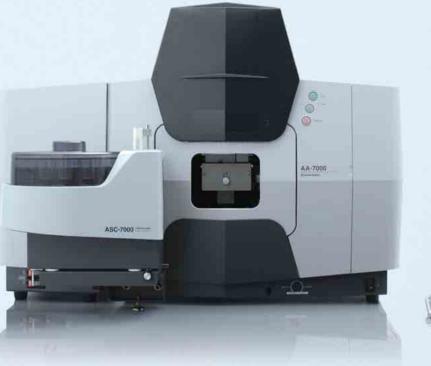





Shimadzu Corporation www.shimadzu.com/an/ Company names, product/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation or its affiliates, whether or not they are used with trademark symbol "TM" or "@". Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services. Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

For Research Use Only. Not for use in diagnostic procedures. The contents of this publication are provided to you "as is" without warranty of any kind, and are subject to change without notice. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication.

> © Shimadzu Corporation, 2014 Printed in Japan 3655-09416-30ANS